COREFORM™

Translucent quartz fiber

GB **INSTRUCTIONS FOR USE** 2

ES **MODO DE EMPLEO** 3

GB

INSTRUCTIONS FOR USE

DESCRIPTION

The transparent COREFORM™, made of clear Polypropylene, are available in five universal sizes to permit easy core build-ups.

Product benefits:

- Transparent material permit light-curing
- Flexible for easy trimming and removing
- Polypropylene will not stick to core material
- Tab on the top to allow pick them up with pliers
- Reference lines every 1mm for accurate contouring
- Number marked for a better recognition of the size

#1	#2	#3	#4	#5
Ø 5	Ø 6,5	Ø 8	Ø 9,5	Ø 10,5
Height = 9,8 mm				

INDICATIONS

COREFORM™ are the ideal disposable matrices for direct core build-up restorations.

PRECAUTIONS

For single use.

No sterile devices.

COREFORM™ cannot be sterilised by autoclave.

STEP-BY-STEP INSTRUCTIONS

1. Select the correct COREFORM™
2. Fill the COREFORM™ your selected composite.
3. Place COREFORM™ over tooth and root canal post.
4. Light-cure if your composite is a light-cured or dual-cured composite.
5. Remove COREFORM™ with a disc or a bur after curing the composite.
6. Finish the preparation in the cervical and occlusal area.

OTHER RECOMMENDATIONS

Cure with double exposure time if a light-cured material is used for optimum results.

SAFETY AND LIABILITY

RTD declines any liability or compensation for possible damage due to:

- use of instruments which do not belong to the system and which may impair the function,
- failure to observe the instructions for use.

The user is responsible for testing the material for its suitability and use for any purpose not explicitly stated in the instructions for use.

For dental use only.

ES

MODO DE EMPLEO

DESCRIPCIÓN

COREFORM™ transparente, hecho de claro de polipropileno, están disponibles en cinco tamaños universales para permitir modelar el muñón.

Beneficios del producto:

- Material transparente que permitan curar de la luz
- Flexible para recorte fácil y quitar
- Polipropileno no se pegue al núcleo material
- Ficha en la parte superior para permitir recoger arriba con las pinzas
- Líneas de referencia de cada 1 mm para contorneado precisa
- Número marcado para un mejor reconocimiento del tamaño

#1	#2	#3	#4	#5
Ø 5	Ø 6,5	Ø 8	Ø 9,5	Ø 10,5
Altura = 9,8 mm				

INDICACIÓN

COREFORM™ son las matrices de uso único ideales para restauraciones de muñón.

PRECAUCIONES DE USO

Para uso único.

No hay dispositivos estériles.

No se recomienda la utilización del autoclave para las COREFORM™.

PREPARACIÓN PASO A PASO

1. Seleccionar la COREFORM™ correcta
2. Llenar le COREFORM™ su composite seleccionado.
3. COREFORM™ lugar más dental y del poste.
4. Fotopolimerizar si su es composite un composite de luz o dual.
5. Quitar COREFORM™ con un disco o una fresa después de curar el composite.
6. Finalizar la preparación en la zona cervical y oclusión.

OTRAS RECOMENDACIONES

Curar con tiempo de exposición doble si se utiliza un material de luz para obtener resultados óptimos.

SEGURIDAD Y RESPONSABILIDAD

RTD declina toda responsabilidad para los daños causados por:

- la utilización de los instrumentos extraños al sistema
- el no seguimiento de las indicaciones marcadas en esta hoja.

Asegurarse que los productos son apropiados para la utilización prevista.

Destinados sólo al uso dental.

- **SUGGESTED SIZE**
- **SUGERENCIAS PARA LA ELECCIÓN DE LA COREFORM™**

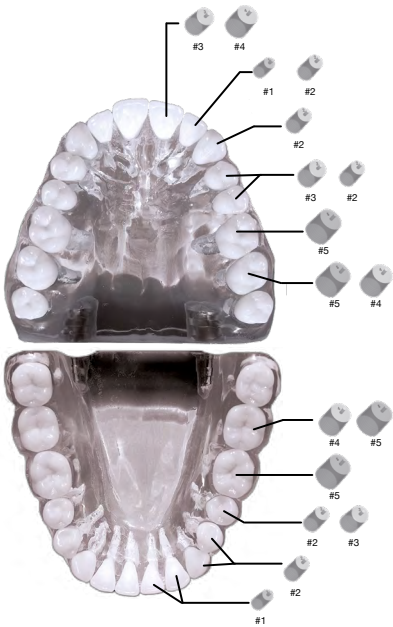

RTD
3 rue Louis Neel
38120 St Egrève Francia

www.rtd.fr
rtd@rtd.fr

-2007-

NOT0940XX00-1107 Rev.: 1107 - 2011 -